

LACTOFERRIN ASSAY

Gastro Health
Marker

The **Diazyme Lactoferrin Assay** is immunoturbidimetric assay used for the quantitative measurement of Lactoferrin in human fecal samples.


Studies have shown that fecal lactoferrin can serve as reliable biomarker, primarily focusing on gastrointestinal health and inflammatory conditions.¹ By quantifying lactoferrin levels in bodily fluids, clinicians can assess the presence and severity of inflammation, particularly in the gastrointestinal tract.²

DIAZYME LACTOFERRIN ASSAY ADVANTAGES

- Particle-enhanced immunoturbidimetric method
- Liquid stable reagent kit, calibrator and control sets offered separately
- Fast test results (10 minutes) for a rapid turnaround time
- Wide range of instrument parameters available for simplifying implementation

REGULATORY STATUS


510(k) Exempt

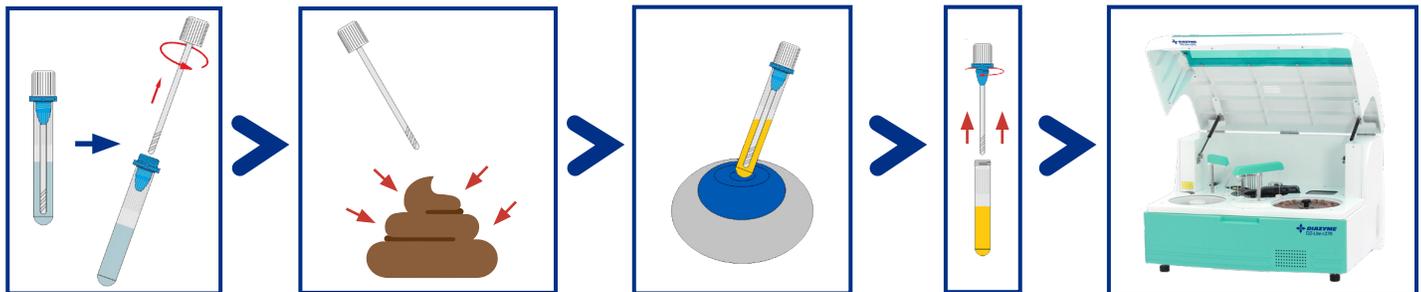

ASSAY SPECIFICATIONS

Method	Particle Enhanced Immunoturbidimetric
Sample Type & Volume	Stool extracts Sample Volume 3 µL
Method Comparison	N: 39 Slope = 0.9 y-intercept = -0.6 R ² = 0.82
Linearity	1.5 to 100 µg/g (AMR)
LOB LOD LOQ	0.5 µg/g 1.006 µg/g 1.5 µg/g
Calibration Levels	6-Point Calibration
Prozone/Hook Tolerance	up to 10,000 µg/g
Reagent On-Board Stability	30 days on-board stability (when stored at 2-8°C)

LACTOFERRIN ASSAY

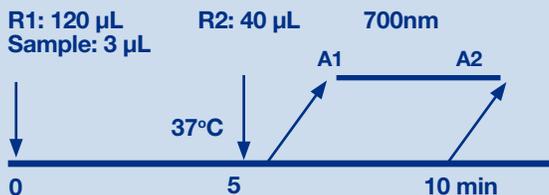

For a list of validated parameters please contact Diazyme technical support at 858-455-4768 or email support@diazyme.com

REFERENCES

1. Yamamoto, Takayuki. "The Clinical Value of Faecal Calprotectin and Lactoferrin Measurement in Postoperative Crohn's Disease." *United European Gastroenterology Journal*, vol. 3, no. 1, 1 Feb. 2015, pp. 5-10. www.ncbi.nlm.nih.gov/pmc/articles/PMC4315679/#:~:br13-2050640614558106.
2. Reenaers C, Bossuyt P, Hindryckx P, Vanpoucke H, Cremer A, Baert F. Expert opinion for use of faecal calprotectin in diagnosis and monitoring of inflammatory bowel disease in daily clinical practice. *United European Gastroenterology Journal*. 2018;6(8):1117-1125. doi:10.1177/2050640618784046

ASSAY PRECISION

The precision of the Diazyme Lactoferrin Assay was evaluated on an AU680 analyzer according to CLSI EP5-A2 guideline. Five samples were tested with 2 replicates with two run per day for 20 days for a total of 80 replicates per sample. Results are summarized below.

Sample	Mean (µg/g)	n	Within Run		Between Run		Between Day		Total	
			SD	CV(%)	SD	CV(%)	SD	CV(%)	SD	CV(%)
1	2.8	80	0.2	8.0	0.2	8.1	0.3	8.9	0.3	12
2	9.0	80	0.4	4.0	0.4	4.2	0.7	7.5	0.8	8.6
3	20.9	80	0.4	1.8	0.8	3.6	0.8	3.7	1.0	4.7
4	45.2	80	1.0	2.2	1.6	3.6	1.6	3.6	2.1	4.7
5	75.9	80	2.3	3.0	2.4	3.2	4.7	6.2	5.2	6.9

ACCURACY & RECOVERY

Five extracted stool samples containing various concentrations of Lactoferrin across the analytical measuring range of the assay were spiked with native Lactoferrin. The stool sample extracts were mixed with the spiking material to add an expected amount of 23 µg/g. Recovery was calculated compared to the baseline result. The spiked sample recoveries were within 10% of the expected values. The results of the recovery study is summarized below.

Specimen Extract	Mean Baseline Result (µg/g)	Spiked Value (µg/g)	Expected Post-Spike Result (µg/g)	Observed Post-Spike Result (µg/g)	Recovery (%)
1	16.7	23	39.7	39.5	99.5
2	26.1	23	49.1	48.9	99.59
3	22.1	23	45.1	44.9	99.56
4	24.1	23	47.1	46.9	99.58
5	37.1	23	60.1	59.9	99.67

DIAZYME LABORATORIES, INC.

12889 Gregg Court, Poway, CA 92064 USA
PO Box 85608, San Diego, CA 92186 USA
Tel: +1-858-455-4768 +1-888-DIAZYME
www.diazyme.com sales@diazyme.com

DIAZYME EUROPE GMBH

Zum Windkanal 21, 01109 Dresden, Germany
Tel: +49-351-886-3300 Fax: +49-351-886-3366
sales@diazyme.de

SHANGHAI DIAZYME CO., LTD.

Building 8, 3879 Dongchuan Road
Minhang District, Shanghai, 200245
Tel: +86-21-54843802 Fax: +86-21-51320663
www.lanyuanbio.com service@lanyuanbio.com